


Quality Control Testing Results – Mitochondrial DNA PCR Reagents  
 October 20 2017

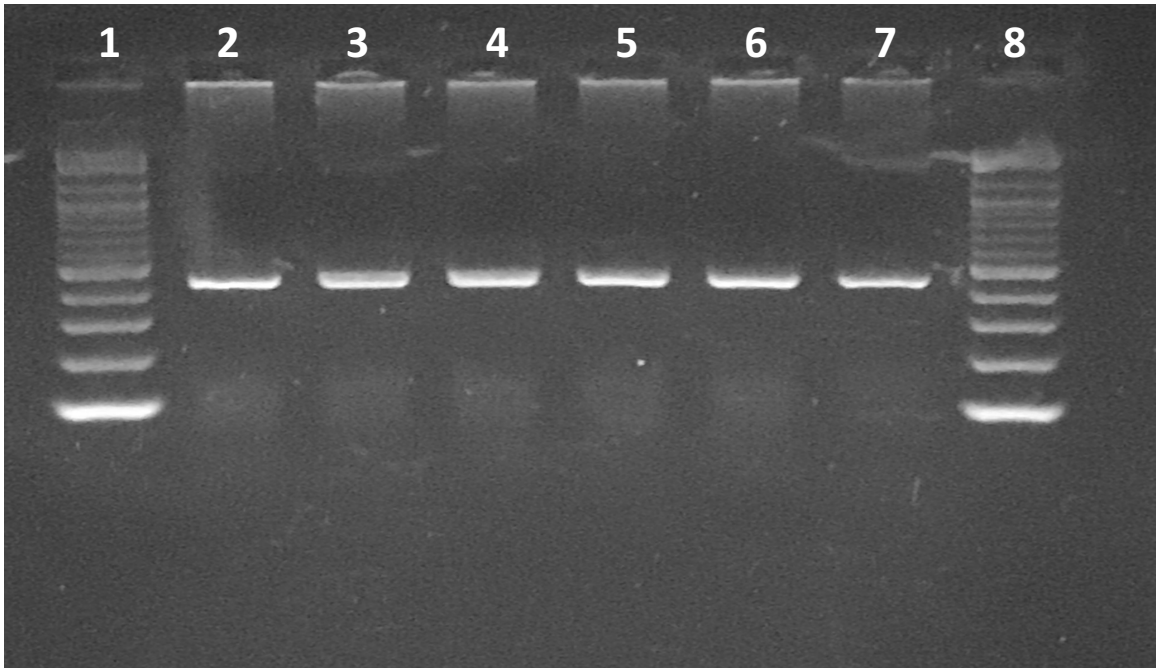

	#1	#2	#3	#4	#5	#6	#7	#8
Master Mix	100 BP Ladder	Lot #01	Lot #01	Lot #01	Lot #01	Lot #01	Lot #01	100 BP Ladder
Primer Mix		Lot #01	Lot #01	Lot #01	Lot #01	Lot #01	Lot #01	
Control DNA		Lot #002	Lot #002	Lot #002	Staff DNA	Staff DNA	Staff DNA	